




Let the iX5™ ClearView™ screen  
help you visualize so you can  
wean patients earlier

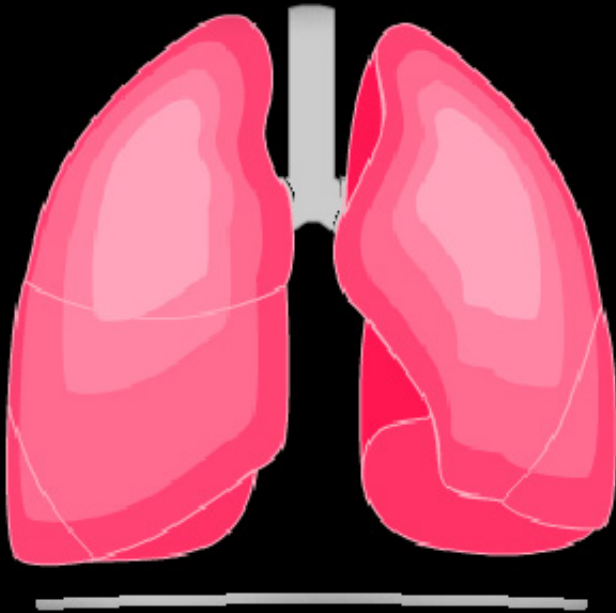


**vyaire**™  
M E D I C A L

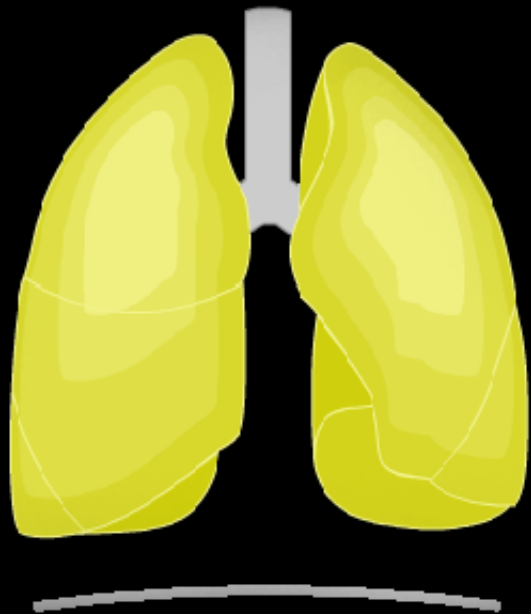

**Know when assisted breathing**

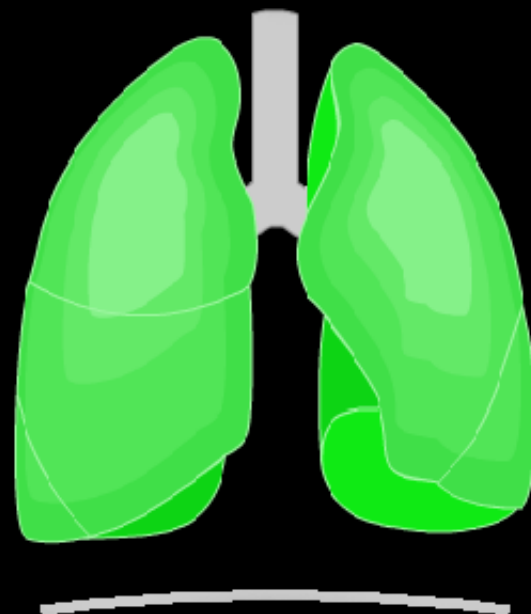

**Turns to spontaneous breathing**

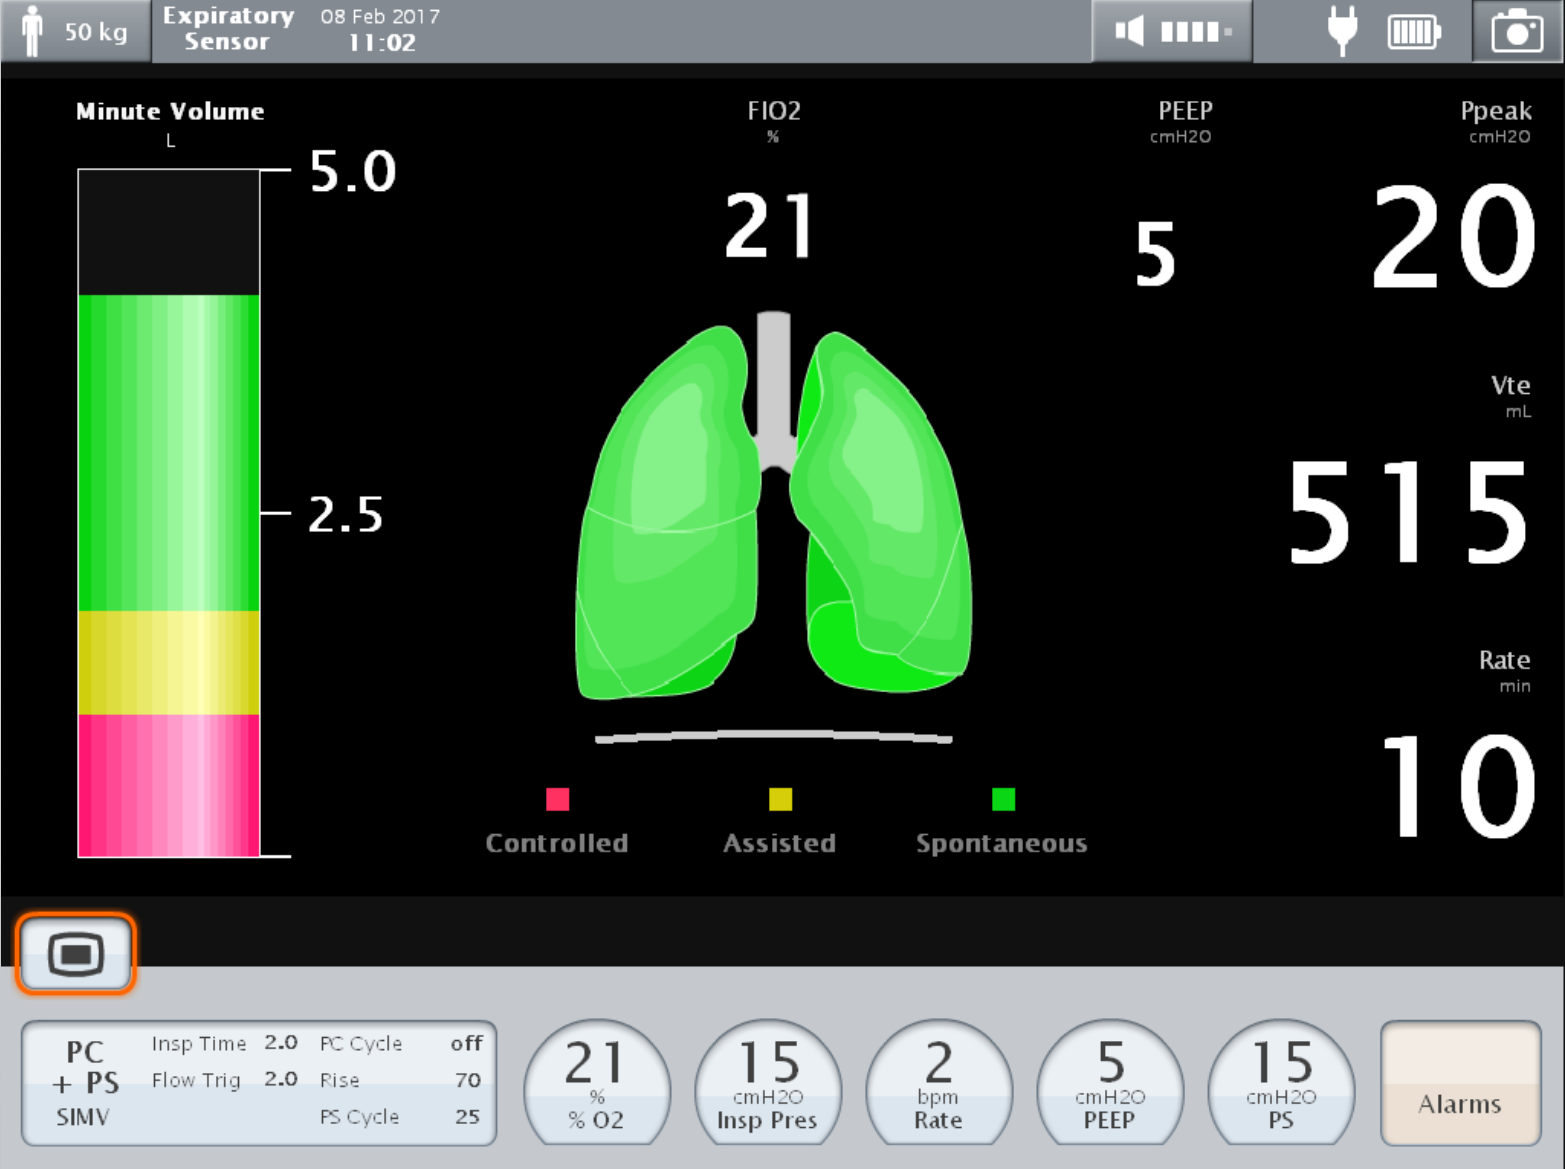

The iX5 ClearView™ screen provides quick clues on patient status that supports early weaning and readiness:

- Minute Volume Bargraph shows portion of the minute volume coming from Controlled, Assisted and Spontaneous Cycles
- Color-coded lung model displaying breath trigger mechanism
- Key patient parameters prominently displayed, enabling remote viewing that facilitates quick patient assessment

Studies have shown that the cost of care increases significantly the longer patients are on a ventilator. Prolonged mechanical ventilation increases median costs by more than \$27,000 per patient and accounts for 64% of total mechanical ventilation costs.<sup>1</sup>

Visit [intl.vyaire.com](http://intl.vyaire.com) to learn more on how the iX5 ClearView user interface can help you and your patients.



## REFERENCES

1. Zilderberg, M., Luppoid, R., Sulsky, S., Shorr, A. Prolonged mechanical ventilation, hospital resource utilization and mortality in the United States. Crit Care Med, March 2008, 36(3):724–730.

## GLOBAL HEADQUARTERS

Vyaire Medical, Inc.  
26125 North Riverwoods Blvd  
Mettawa, IL 60045  
USA



OBELIS S. A  
Bd General Wahis, 53  
1030, Brussels  
BELGIUM



Intermed Equipamento Médico  
Hospitalar Ltda  
CNPJ: 49.520.521/0001-69  
I.E.: 278.082.665-115  
Rua Santa Mônica, 980  
Parque Industrial San José  
06715-856, Cotia/SP, BRAZIL



## [vyaire.com](http://vyaire.com)

### For Global distribution.

The iX5 is not available for sale in the US and may not be available in every region, please contact a Vyaire representative for availability.

© 2020 Vyaire. Vyaire, the Vyaire logo and all other trademarks or registered trademarks are property of Vyaire Medical, Inc., or one of its affiliates. Please read the complete Instructions For Use that come with the devices or follow the instructions on the product labelling. VYR-INT-2000085